


Aprovecho Research Center

Advanced Studies in Appropriate Technology Laboratory


79093 Highway 99, PO Box 1175
Cottage Grove, Oregon 97424 USA

541-767-0287
www.aprovecho.org

Bill's Personal IAP Exposure During Stove Camp.....

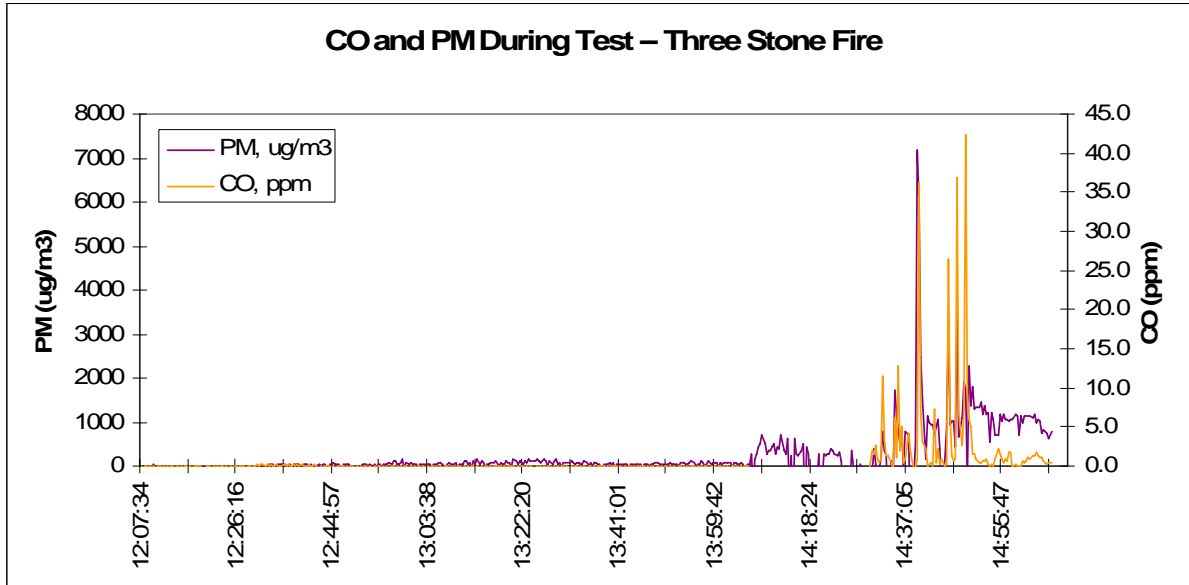

Average PM During Test = 913 $\mu\text{g}/\text{m}^3$ Average CO During Test = 3.2 ppm

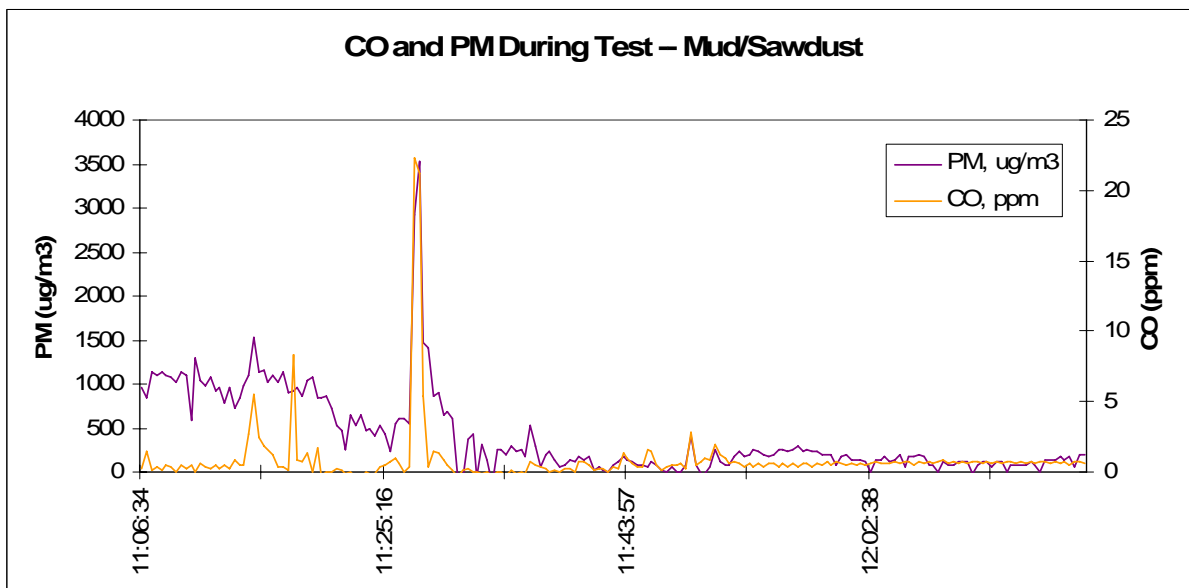

Average PM During Test = 485 $\mu\text{g}/\text{m}^3$ Average CO During Test = 1.0 ppm